

T34 Syringe Driver

Information for patients and carers

Palliative Care

Patient Information Leaflet


What is a syringe driver?

A syringe driver is a small, portable, battery operated device which administers medicine directly under the skin. Medication is pumped continuously over a 24 hour period.

A syringe driver consists of:

- The machine
- Syringe (which contains medication)
- Tubing with a soft, thin, plastic needle at the end
- Plastic locked box

The soft, plastic needle of the syringe driver is inserted just under the skin on the chest, abdomen, top of the arm or top of the leg and once inserted, cannot be felt (see picture below)

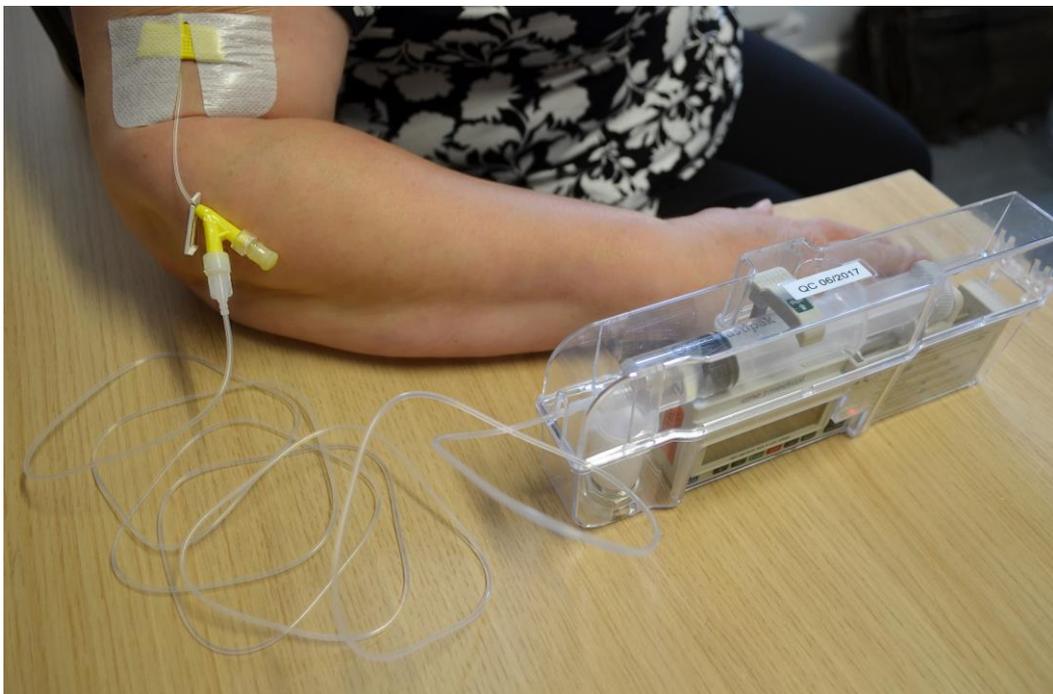

How will a syringe driver help?

The syringe driver is designed to give medication over 24 hours and is often used to control symptoms such as pain, vomiting and breathlessness, when there is difficulty swallowing tablets and/or to avoid multiple injections.

Each day the syringe driver will be checked by a nurse and a new syringe containing medication will be attached. Your symptoms will be regularly reviewed and your medication adjusted accordingly.

It is common for there to be more than one medication in the syringe at a

time. Additional doses of medicines may be given if required.

The length of time a syringe driver is needed is individual to each patient.

It is important that you let your doctor or nurse know if your symptoms are not controlled, or if new symptoms develop.

Sometimes people use a syringe driver for a short time and are then able to take medication by mouth again.

How will a syringe driver affect daily routine?

The syringe driver should not restrict most day to day activities, but there are some things to consider/avoid:

Bathing:

- If the syringe driver gets wet it will not work and the needle site needs to remain dry. Please seek advice from the nursing team who will need to apply a waterproof dressing over the needle site and give advice on how to keep the syringe driver dry and safe during bathing/showering. (This will be dependent on the facilities available in hospital or in your home).

Going out:

- The syringe driver can be carried in a bag.
- Advice from a doctor should be sought before driving.

Eating:

- There are no specific restrictions on what you can eat or drink, unless there are particular instructions from your doctor.

Heat:

- If the syringe driver were to become too warm, this can affect the medication in it; avoid putting it near extra heat sources such as a heat pad, hot water bottle, electric blanket, or in direct sunlight.

Holidays:

- Professional nursing support would be required if planning to be away for more than 24 hours. District Nursing teams outside the local area may be able to assist if planned in advance. Liaison with the local GP practice would be needed.

Clothes:

- There are no specific restrictions so long as the clothing does not impede access to the syringe driver and the needle site is easily accessed (e.g. loose clothing and, for example a cardigan would be easier to remove than a jumper).

Troubleshooting

Syringe driver alerts:

The syringe driver is a very reliable machine. If there are any problems or faults an alarm will sound and there will be an LCD screen message displayed which will indicate what the problem is.

For example:

- Low battery
- Occlusion (twisted/kinked tubing)
- Syringe displacement
- Clouding or sediment in the syringe

In all cases the nursing team is responsible for ensuring the syringe driver is working effectively. In hospital it will be regularly checked and at home it will be checked every day. However, if problems arise between nurse visits you do not need to do anything apart from informing your nurse right away; you will have been provided with 24 hour contact numbers.

Please do not interfere with the line or pump, and do not press the buttons on the control panel.

Damage:

A syringe driver in its protective box is quite strong, but if it were to be

dropped or crushed please inform the nursing team who can ensure it is still working, or replace it if not.

Things to look out for:

If the skin around the needle becomes red, swollen or painful, the nursing team need to be notified and they will arrange to remove the needle and replace it with a new one in a new site.

If the syringe driver has been exposed to heat, i.e. accidental exposure to the sun, inform the nursing team as this can compromise the effectiveness of the medication.

Leaflet Details

Approved by: PD & ILG
Date of Publication: 16/08/2017
Reference Number: PIL/061
Author: Palliative Care Team
Review Date: 01/08/2020



Other formats

If you would like to receive this information in an alternative format, then please contact : 01539 795497

Travelling to our hospitals

For the best way to plan your journey visit our website:
<http://www.UHMB.nhs.uk/> or contact Patient Advice and Liaison Service (PALS): 01539 795497

Useful Contact Details

NHS 111 (for 24 hour urgent health advice): telephone 111

Your Information

If you would like to know how we use, share, disclose and secure your information and your rights of access to the information we hold about you, visit the Trust's website: <http://www.UHMB.nhs.uk/> or contact Patient Advice and Liaison Service (PALS) on 01539 795497.

Evidence

Details of the evidence used in writing this leaflet are available on request from: Patient Information Officer at 01524 512476.

Feedback

We appreciate and encourage feedback. If you need advice or are concerned about any aspect of care or treatment, please speak to a member of staff or contact PALS on 01539 795497.

UHMBT is a no smoking Trust. Smoking is not permitted on any of the hospital sites. You can contact the NHS North Lancashire Stop Smoking services on the number below:

NHS Quit Squad - **0800 328 6297**

If you live in Cumbria, please call **0300 013 3000** to find a local pharmacy who are offers 1-2-1 support and nicotine replacement therapy.

University Hospitals of Morecambe Bay Trust: a great place to be cared for; a great place to work.